

March 8, 1999

0306
Dr. Stephen C. Erfurth
Oregon Medical Laboratories
722 East 11th Avenue
Eugene, OR 97401

Dear Dr. Eurfurth:

The enclosed critique was developed from the inspection reports of the inspectors who conducted the fifteenth maintenance inspection of your laboratory under the National Laboratory Certification Program (NLCP). Based upon our review of these reports, the laboratory's performance in this inspection is highly acceptable.

RTI is recommending to the Department of Health and Human Services (HHS) that the laboratory's certification be continued based upon its acceptable performance in the inspection phase of the program. The laboratory must review the enclosed critique and take all necessary corrective actions. All corrective actions must be implemented within 30 days of receipt of this correspondence. It is not necessary for the laboratory to submit a written response to RTI. All corrective actions will be reviewed during the next inspection.

If you have any questions or if we can be of further assistance, please call me at (919) 541-7265 or Dr. Michael Baylor at (919) 541-7043.

Sincerely,

Deborah J. Denson NLCP Inspection Analyst

Deborah of Denson


Enclosure

CC:

Project Files/M15

Dr. David Kuntz

Dr. Robert Pick





Document Review and Critique

Laboratory I.D. Number: <u>0306</u>
Document No. Final

Laboratory:

Oregon Medical Laboratories

Location:

Eugene, OR

Document Reviewed:

[] Application Form
[XX] Inspection Report #M15
[] Other

Date. 4 February 1999

Status:

[XX] Highly Acceptable

[] Unacceptable

] Acceptable] Failure


A review of the National Laboratory Certification Program (NLCP) inspection reports has been completed. It is the judgment of the reviewers that the laboratory has met the standards required for the inspection phase of the Program.

There were a number of comments and observations generated as a result of the inspection that are detailed on the following pages for the attention of the laboratory before its next inspection.

NLCP • Research Triangle Institute

Page 1

Section E. Standard Operating Procedures - Procedures Manual

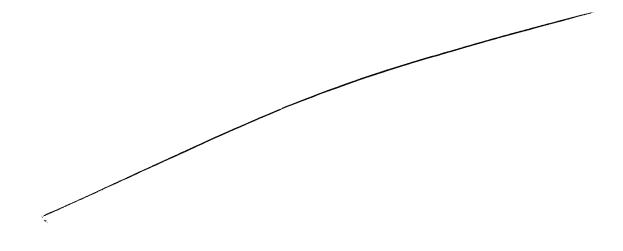

Section F. Chain-of-Custody, Accessioning, and Security

Section G. Quality Control

Section H. Initial Tests

Section I. Confirmatory Tests

Section J. Records Audit

Section K. Reporting

Section L. Computers, Software, and LIMS

Section M. Equipment and Maintenance






September 10, 1999

0306
Dr. Stephen C. Erfurth
Oregon Medical Laboratories
722 East 11th Avenue
Eugene, OR 97401

Dear Dr. Erfurth:

The enclosed critique was developed from the inspection reports of the inspectors who conducted the sixteenth maintenance inspection of your laboratory under the National Laboratory Certification Program (NLCP). Based upon our review of these reports, the laboratory's performance in this inspection is highly acceptable. However, the laboratory must take steps to correct/clarify the following issues raised:

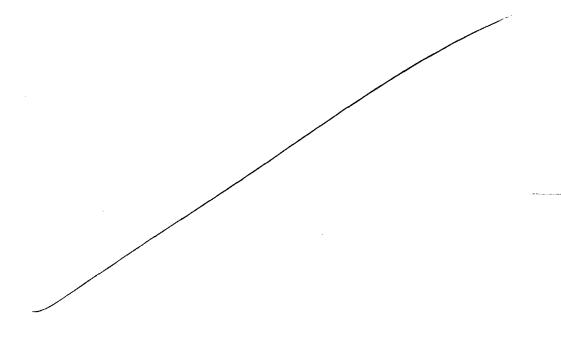



RTI is recommending to the Department of Health and Human Services (HHS) that the laboratory's certification be continued based upon its acceptable performance in the inspection phase of the program. The laboratory must take steps to correct the issues cited above. The laboratory must also review the enclosed critique and take all necessary corrective actions. All corrective actions must be implemented within 30 days of receipt of this correspondence. It is *not necessary* for the laboratory to submit a written response to RTI. All corrective actions will be reviewed during the next inspection.

If you have any questions or if we can be of further assistance, please call me at (919) 541-6176 or Dr. Michael Baylor at (919) 541-7043.

Sincerely,

Susan Crumpton

NLCP Inspection Analyst

Enclosure


cc: Project Files/M16

Document Review and Critique Laboratory I.D. Number: 0306 Document No. Final **Oregon Medical Laboratories** Laboratory: Eugene, OR Location: **Document Reviewed:**] Application Form [XX] Inspection Report #M16 Date: 12 August 1999 [] Other____ Status: [XX] Highly Acceptable] Acceptable [] Unacceptable] Failure

A review of the National Laboratory Certification Program (NLCP) inspection reports has been completed. It is the judgment of the reviewers that the laboratory has met the standards required for the inspection phase of the Program.

There were a number of comments and observations generated as a result of the inspection that are detailed on the following pages for the attention of the laboratory before its next inspection.

Section E. Standard Operating Procedures - Procedures Manual

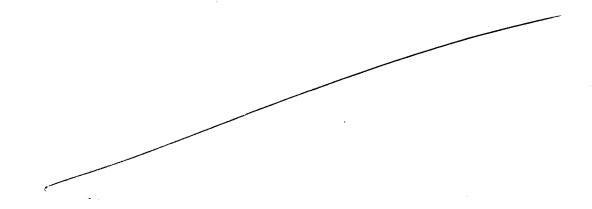


Section F. Chain-of-Custody, Accessioning, and Security

Section G. Quality Control

Section H. Initial Tests

Section I. Confirmatory Tests

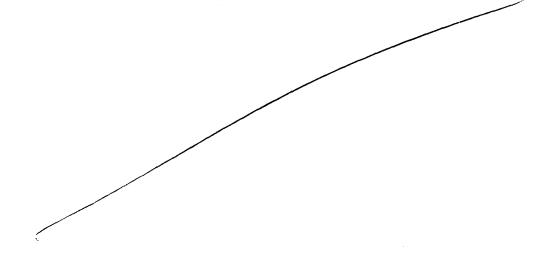

Section J. Records Audit

Section K. Reporting

Section L. Computers, Software, and LIMS

\/er	Final
vei.	1 11 141

Lab ID# 0306

Section M. Equipment and Maintenance



March 3, 2000

0306
Dr. Stephen C. Erfurth
Oregon Medical Laboratories
722 East 11th Avenue
Eugene, OR 97401

Dear Dr. Erfurth:

The enclosed critique was developed from the inspection reports of the inspectors who conducted the seventeenth maintenance inspection of your laboratory under the National Laboratory Certification Program (NLCP). Based upon our review of these reports, the laboratory's performance in this inspection is highly acceptable. The inspection team had some areas of concern, which are detailed in the attached critique.

RTI is recommending to the Department of Health and Human Services (HHS) that the laboratory's certification be continued based upon its acceptable performance in the inspection phase of the program. The laboratory must review the enclosed critique and take all necessary corrective actions. All corrective actions must be implemented within 30 days of receipt of this correspondence. It is *not necessary* for the laboratory to submit a written response to RTI. All corrective actions will be reviewed during the next inspection.

If you have any questions or if we can be of further assistance, please call me at (919) 541-7265 or Dr. Michael Baylor at (919) 541-7043.

Sincerely,

Deborah J. Denson NLCP Inspection Analyst

Deborah Jlenso

Enclosure

cc: Project Files/M17



Document Review and Critique

Laboratory I.D. Number: 0306

Document No. Final

Laboratory:

Oregon Medical Laboratories

Location:

Eugene, OR

Document Reviewed:

[] Application Form

[XX] Inspection Report #M17

Date: 3 February 2000

[] Other _

Status:

[XX] Highly Acceptable


] Unacceptable

] Acceptable] Failure

A review of the National Laboratory Certification Program (NLCP) inspection reports has been completed. It is the judgment of the reviewers that the laboratory has met the standards required for the inspection phase of the Program.

There were a number of comments and observations generated as a result of the inspection that are detailed on the following pages for the attention of the laboratory before its next inspection.

Section E. Standard Operating Procedures - Procedures Manual

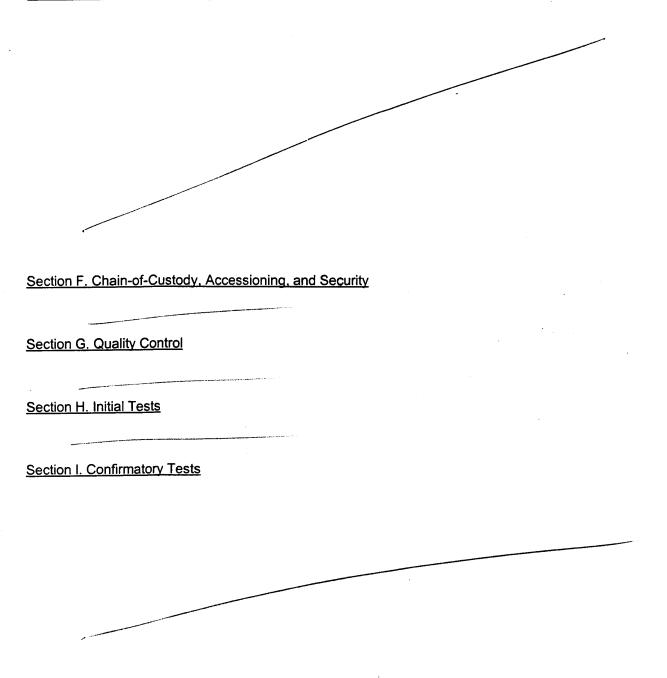

Section J. Records Audit

Section K. Reporting

Section L. Computers, Software, and LIMS

Section M. Equipment and Maintenance




September 19, 2000

0306 Dr. Stephen C. Erfurth Oregon Medical Laboratories 722 East 11th Avenue Eugene, OR 97401

Dear Dr. Erfurth:

The enclosed critique was developed from the inspection reports of the inspectors who conducted the eighteenth maintenance inspection of your laboratory under the National Laboratory Certification Program (NLCP). Based upon our review of these reports, the laboratory's performance in this inspection is highly acceptable. The inspection team had some areas of concern, which are detailed in this cover letter and attached critique.

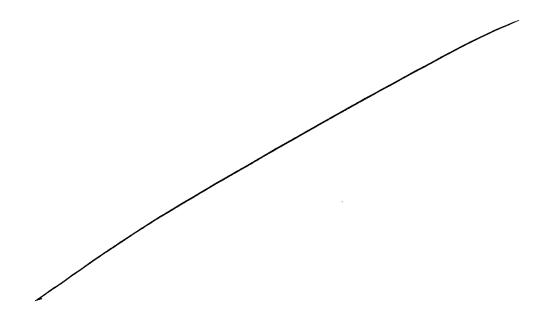



RTI is recommending to the Department of Health and Human Services (HHS) that the laboratory's certification be continued based upon its acceptable performance in the inspection phase of the program. The laboratory must take steps to correct the issues cited above. The laboratory must also review the enclosed critique and take all necessary corrective actions. All corrective actions must be implemented within 30 days of receipt of this correspondence. It is *not necessary* for the laboratory to submit a written response to RTI. All corrective actions will be reviewed during the next inspection.

If you have any questions or if we can be of further assistance, please call me at (919) 541-6176 or Dr. Michael Baylor at (919) 541-7043.

Sincerely,

Susan Crumpton

NLCP Technical Analyst

Enclosure

cc: Project Files/M18

Document Review and Critique

Laboratory I.D. Number: 0306

Document No. Final

Laboratory:

Oregon Medical Laboratories

Location:

Eugene, OR

Document Reviewed:

] Application Form

[XX] Inspection Report #M18
[] Other _____

Date: 3 August 2000

Status:

[XX] Highly Acceptable


Unacceptable

] Acceptable] Failure

A review of the National Laboratory Certification Program (NLCP) inspection reports has been completed. It is the judgment of the reviewers that the laboratory has met the standards required for the inspection phase of the Program.

There were a number of comments and observations generated as a result of the inspection that are detailed on the following pages for the attention of the laboratory before its next inspection.

Section E. Standard Operating Procedures - Procedures Manual

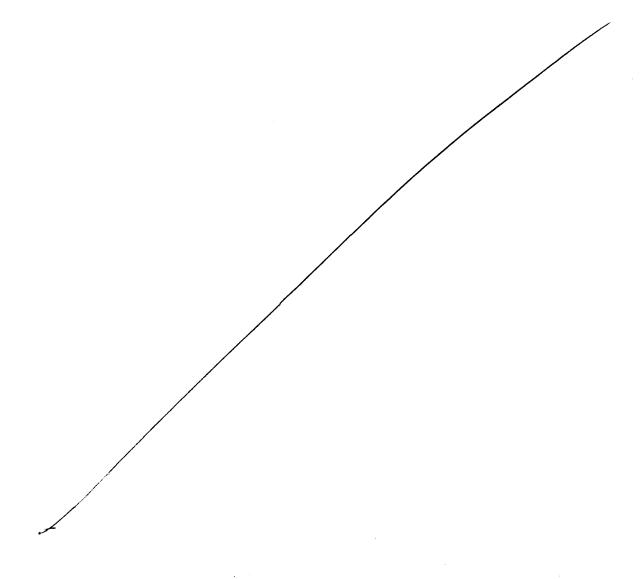

Section F. Chain-of-Custody, Accessioning, and Security

Section G. Quality Control

Section H. Initial Tests

Section I. Confirmatory Tests

Section J. Records Audit

Section K. Reporting

Section L. Computers, Software, and LIMS

Section M. Equipment and Maintenance